

APPENDIX

10. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

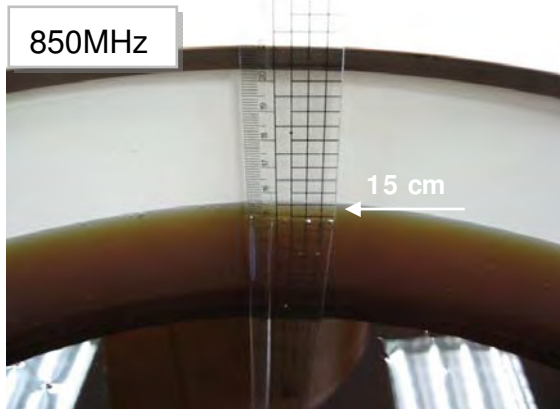


Fig.2.1

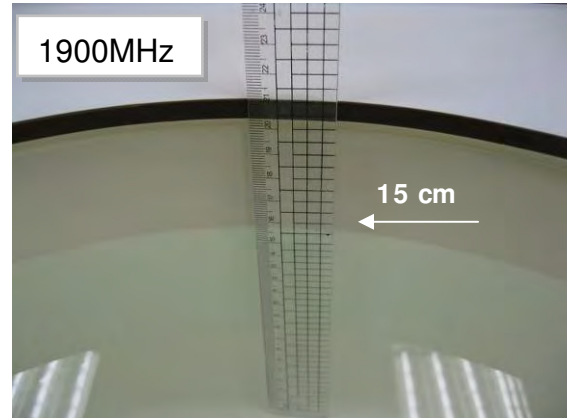


Fig.2.2

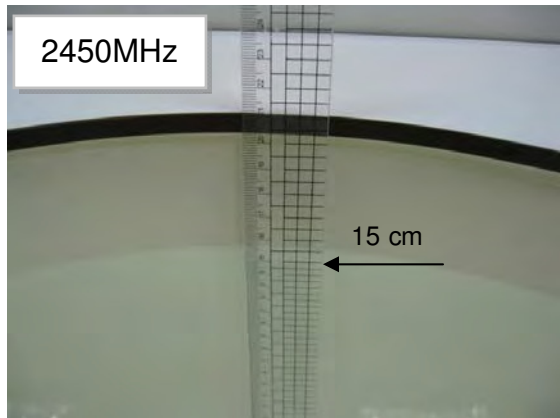


Fig.2.3

Body - distance between flat phantom and EUT is 5 mm

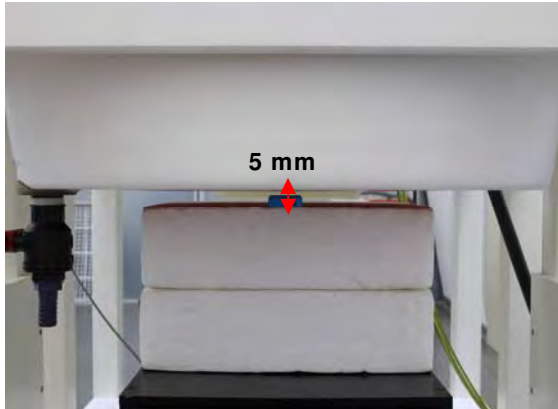


Fig.3 EUT Back side to flat phantom

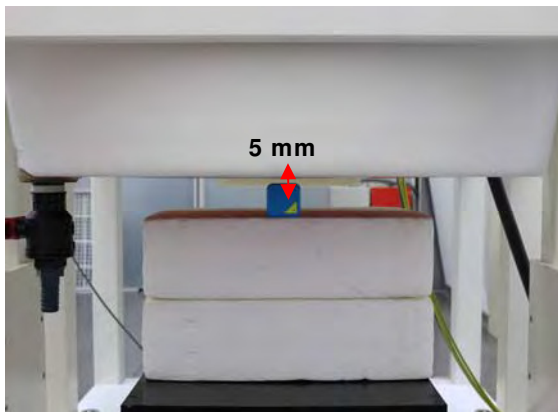


Fig.4 EUT Bottom side to flat phantom


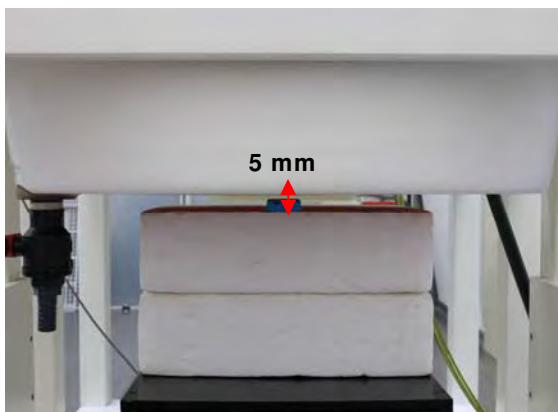


Fig.5 EUT Front side to flat phantom

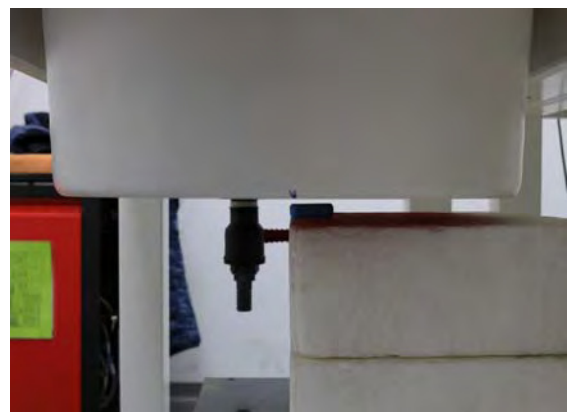

Body - distance between flat phantom and EUT is 5 mm

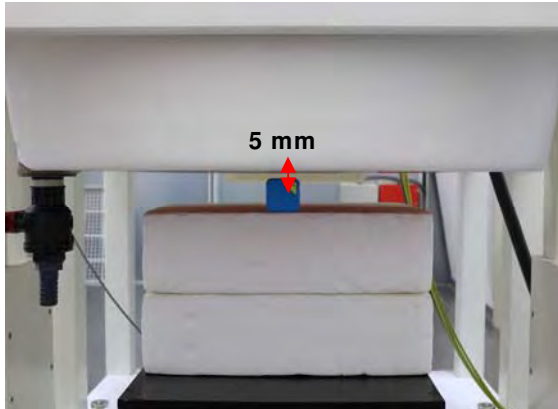


Fig.6 EUT Left side to flat phantom



Fig.7 EUT Right side to flat phantom


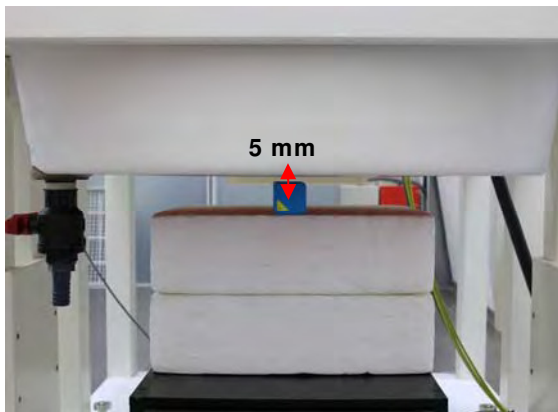


Fig.8 EUT Top side to flat phantom

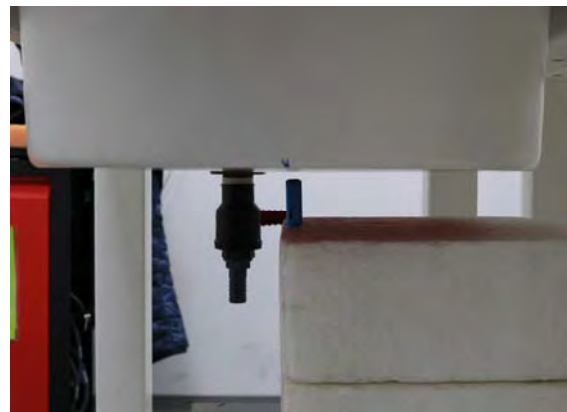

11. Photographs of the EUT

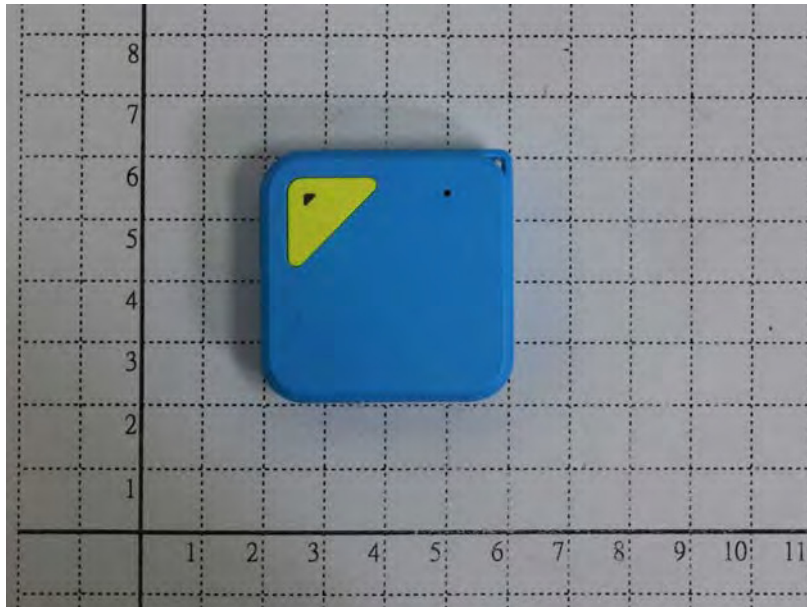


Fig.9 Front view of EUT

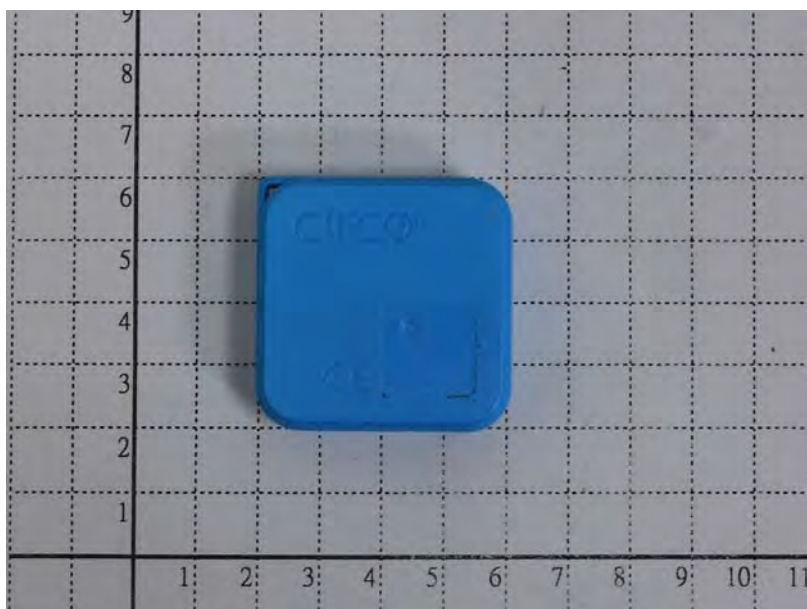


Fig.10 Back view of EUT



Fig.11 Antenna position of EUT

- End of Report -